

The ibidi labware is comprised of a variety of μ-Slides, μ-Dishes, and μ-Plates, which have all been designed for high-end microscopic analysis of fixed or living cells. The glass bottom versions are especially designed for TIRF, super-resolution, and single molecule applications. The μ-Slide 8 Well<sup>high</sup> Glass Bottom is a chambered coverslip with 8 wells for convenient cell culture, immunofluorescence, and high-end microscopy. The slide is intended for the optimization of experimental parameters, such as antibody dilution, seeding density, or drug concentration.

This document applies to the following product:

80807 **μ-Slide 8 Well<sup>high</sup> Glass Bottom**

## Material

The μ-Slide 8 Well<sup>high</sup> Glass Bottom is made with a glass coverslip bottom. It is not possible to detach the bottom from the upper part. The slide is intended for one-time use and is not autoclavable, since it is only temperature-stable up to 80 °C/175 °F.

### Optical Properties of Glass Coverslip

Refractive index	1.523
Abbe number	55
Thickness	No. 1.5H (170 μm ± 5 μm)
Material	Schott borosilicate glass, D 263 M




**CAUTION** – Be cautious when handling ibidi labware products with a glass bottom! The glass coverslip or slide is fragile and can break easily. Handle these items carefully to prevent physical injury and damage to devices due to medium leakage.

## Geometry

The μ-Slide 8 Well<sup>high</sup> Glass Bottom provides a standard slide format according to ISO 8037/1.

### Specifications

Outer dimensions (w × l)	25.5 × 75.5 mm <sup>2</sup>
Number of wells	8
Dimensions of wells (w × l × h)	9.4 × 10.7 × 9.3 mm <sup>3</sup>
Volume per well	300 μl
Height with/without lid	10.8 / 9.5 mm
Growth area per well	1.0 cm <sup>2</sup>
Coating area per well	2.2 cm <sup>2</sup>
Bottom	Glass Bottom

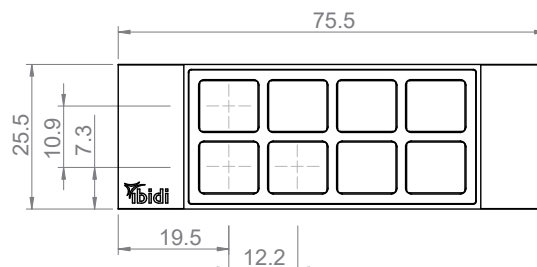

## Shipping and Storage

This product is sterilized and sealed in a gas-permeable packaging. The shelf life under proper storage conditions (in a dry place, no direct sunlight) is outlined in the following table.

Conditions	
Shipping conditions	Ambient
Storage conditions	RT (15–25°C)

Shelf Life	
Glass Bottom	36 months

## Surface

The μ-Slide 8 Well<sup>high</sup> Glass Bottom is manufactured with a glass coverslip. Washing it (e.g., with PBS) before cell seeding helps removing glass dusts, which enhances direct cell growth on the surface.

## Coating

Detailed information about coatings is provided in [Application Note 08: Coating Protocols for ibidi Labware](#).

In short, specific coatings are possible following this protocol:

1. Prepare your coating solution according to the manufacturer's specifications. Adjust the concentration to a coating area of 2.2 cm<sup>2</sup> and a volume of 300 μl per well.
2. Apply 300 μl per well and leave it at room temperature for at least 30 minutes.
3. Aspirate the solution and wash with the recommended protein dilution buffer.
4. The coated slide is ready to be used. Be aware that allowing the coated surface to dry out is not recommended, as some coating proteins may degrade upon drying.

## Seeding Cells

1. Trypsinize and count the cells as usual. Dilute the cell suspension to the desired concentration. Depending on your cell type, application of a  $5\text{--}11 \times 10^4$  cells/ml suspension should result in a confluent layer within 2–3 days.
2. Apply 300 μl cell suspension per well. Avoid shaking, as this will result in inhomogeneous cell distribution.
3. Cover the slide with the supplied lid. Incubate as usual (e.g., at 37°C and 5% CO<sub>2</sub>).

Insensitive cells can be left in their seeding medium for several days and grow to confluence there. However, optimal results might be achieved when the medium is changed every 2–3 days. For this, carefully aspirate the old medium and replace it by 300 μl fresh medium per well.

## Microscopy

To image your cells, no special preparations are necessary. Living or fixed cells can be directly observed, preferably on an inverted microscope. The bottom cannot be removed. For optimal results in fluorescence microscopy and for storage of fixed and stained samples, ibidi provides mounting media that are optimized for ibidi labware:

Cat. No. 50001: [ibidi Mounting Medium](#)

Cat. No. 50011: [ibidi Mounting Medium with DAPI](#)



**TIP** – A bent meniscus at the air-liquid interphase in small open wells will destroy the phase contrast effect of your microscopy image. Use the ibidi Ph<sup>+</sup> slides or channel slides to overcome this disturbing effect.

## Immersion Oil

When using ibidi Glass Bottom products with oil immersion objectives, there is no known incompatibility with any immersion oil on the market. All types of immersion oils can be used.

## Chemical Compatibility

The following table provides basic information on the chemical and solvent compatibility of the μ-Slide 8 Well<sup>high</sup> Glass Bottom. For a full list of compatible solvents and more information on chemical compatibility, visit [ibidi.com/chemicals](https://www.ibidi.com/chemicals).

Chemical / Solvent	Compatibility
Methanol	Yes
Ethanol	Yes
Formaldehyde	Yes
Acetone	No
Mineral oil	Yes
Silicone oil	Yes
Immersion oil	See Section "Immersion Oil"

## For research use only!

Further information can be found at [ibidi.com](https://www.ibidi.com). For questions and suggestions, please contact us by e-mail at [info@ibidi.com](mailto:info@ibidi.com) or by telephone at +49 (0)89/520 4617 0.  
© ibidi GmbH, Lochhamer Schlag 11, 82166 Gräfelfing, Germany.